




Agilent Technologies

alcool organomagnésien

Sample ID:2021-11-10T17-45-59

Sample Scans:16
Background Scans:16
Resolution:2
System Status:Bon
File Location:C:\Users\Public\Documents\Agilent\MicroLab\Results\2021-11-10T17-45-59.a2r

Method
Name:C:\Users\Public\Documents\Agilent\MicroLab\Methods\Agreg.a2m
User:ens
Date/Time:11/10/2021 5:45:59
Range:4000 - 650
Apodization:Happ-Genzel

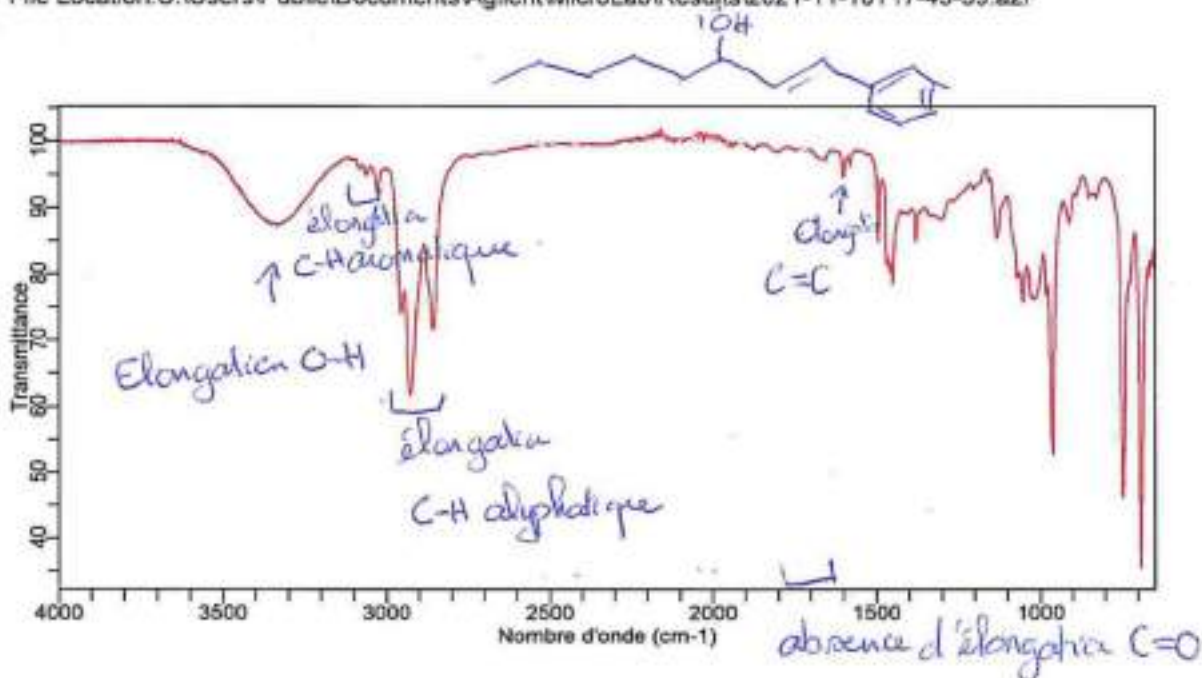

Peak Number	Wavenumber (cm ⁻¹)	Intensity
-------------	--------------------------------	-----------